

mini

OPERATIONS MANUAL

R*hapsody*
[with BluWave™ SP]



MINI BEHIND-THE-EAR

Table of Contents

Identification

Features, Controls and Identification	2
---	---

Preparation

Batteries	4
-----------------	---

Battery Indicator Tones.....	6
------------------------------	---

Tamper Resistant Battery Compartment	7
--	---

Insertion and Removal

Custom Earmold	10
----------------------	----

Instant Fit Earbud or Custom Eartip	13
---	----

Operation

On, Off and Volume Levels	16
---------------------------------	----

Multimemory Settings	17
----------------------------	----

Directional Settings	18
----------------------------	----

Telephone Use.....	19
--------------------	----

Self Check.....	21
-----------------	----

Summary of Settings	22
---------------------------	----

Hearing System Care

Instrument Care.....	24
----------------------	----

Standard Tubing Care	24
----------------------------	----

Thin Tubing Care	26
------------------------	----

Service and Repair.....	29
-------------------------	----

Troubleshooting Guide	30
-----------------------------	----

Tips for Better Communication

For You	32
---------------	----

For Your Family and Friends.....	33
----------------------------------	----

FDA Information

Required Information	36
----------------------------	----

Identification

Features, Controls and Identification

Your hearing system controls include:


1. Earhook and Comfort Fit Solutions
2. Microphone(s)
3. Multimemory button
4. Battery compartment (on/off control)
5. Side indicator **RED** is for **RIGHT** ear,
BLUE is for **LEFT** ear.
6. Tamper resistant battery compartment lock

Your hearing system can be identified by:


7. Location of serial number
8. Location of manufacturer's name and model name

Comfort Fit Solutions:



9. Standard Earmold with tubing
10. Thin tube with Instant Fit Earbud
11. Thin tube with Custom Eartip

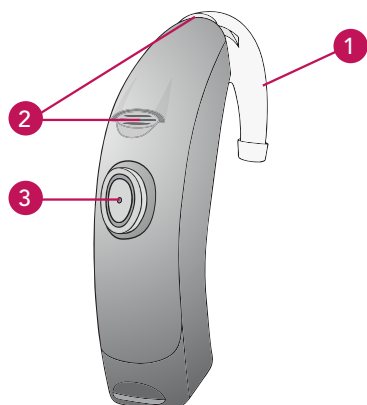

9

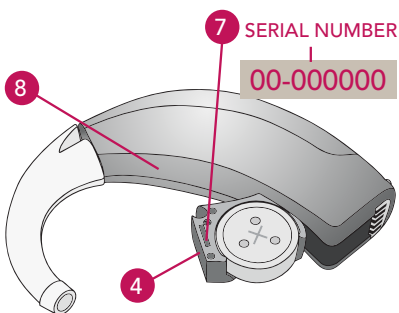

10



11

Preparation


Batteries

Your hearing system uses a size 312 battery as its power source. This battery size can be identified by the brown color code on the packaging.




To insert or replace the battery:


1. Use the nail grip on the battery door.
2. Open the battery door gently and remove the old battery.
3. Remove the tab from the new battery.
4. Line up the battery's plus "+" sign (flat side of the battery) with the "+" on the battery door.
5. Close the battery door.




1




2



3



4



5

Preparation

Battery Indicator Tones

An indicator will sound when the battery's voltage is low. You have approximately 20 minutes* to replace the battery. A different tone lasting two seconds will sound just before the battery stops working.


** Actual time between low battery indicator and shut down will vary depending on environmental noise levels and brand of battery used.*

Preparation

Tamper Resistant Battery Compartment

To lock the battery door:


Use an appropriate tool to slide the recessed switch to the left until it "clicks" and the colored mark is visible.



To unlock the battery door:

Slide the recessed switch to the right until it "clicks" and the colored mark disappears.

Locking the door is not necessary for operation.



Preparation





Helpful Hints

- NEVER FORCE THE DOOR SHUT; this could result in serious damage; if the door will not close securely, check that the battery is inserted correctly
- Do not open the battery door too far or damage is likely to occur
- Dispose of used batteries immediately in the proper waste or recycling container
- Because batteries can vary in size and performance, your hearing care professional is your best source for lifespan estimates and verification that you are using the proper size and type

 **WARNING:**

**HEARING INSTRUMENT BATTERIES ARE
DANGEROUS IF SWALLOWED.**

**National Button Battery
Ingestion Hotline (202) 625-3333**

-  Keep out of reach of children and pets
-  Check your medications before taking them – batteries have been mistaken for pills
-  Never put batteries in your mouth, as they can easily be swallowed
-  National Button Battery Ingestion Hotline:
202-625-3333

Insertion and Removal

Custom Earmold


To insert the Custom Earmold and hearing instrument:

1. Hold the Custom Earmold with your thumb and forefinger on the outer side near the tubing.
2. Tilt your hand slightly forward and gently insert the canal tip of the Custom Earmold into your ear canal.
3. Rotate the Custom Earmold backwards.
4. Softly press the Custom Earmold into place with your fingertip.
5. Carefully place the BTE behind your ear wrapping the earhook over the top of your ear.


To remove the hearing instrument and Custom Earmold:

Take the instrument from behind your ear and gently pull the Custom Earmold outward. Pulling lightly down on the ear lobe may help loosen the Custom Earmold as it is removed.


Insertion and Removal




1




2




3



4



5



Insertion and Removal


Helpful Hints

- Minor irritation and inflammation may occur as your ear becomes accustomed to having an object in it; if so, please contact your hearing care professional.
- If an actual allergic reaction occurs, alternative earmold materials are available; contact your hearing care professional.
- Severe swelling, discharge from the ear, excessive wax, or other unusual conditions warrant immediate consultation with a physician.


Insertion and Removal of Instant Fit Earbud or Custom Eartip

To insert the Instant Fit Earbud or Custom Eartip:


1. Insert the Instant Fit Earbud/Custom Eartip into your ear canal.
2. Gently wrap the BTE over your ear until it rests securely behind your ear.
3. Place the earlock in the concha of your ear.



1



2




3


Insertion and Removal

To remove the hearing instrument and Instant Fit Earbud:


1. Remove the lock from the concha bowl of your ear.
2. Remove the hearing instrument from behind your ear.
3. Gently grasp the tubing at the opening of the ear canal and pull outward.



1




2




3

To remove the hearing instrument and Custom Eartip:


1. Remove the lock from the concha bowl of your ear.
2. Remove the hearing instrument from behind your ear.
3. Grasp the removal line on the Custom Eartip and gently pull outward.



1



2



3

Operation

On, Off and Volume Levels

To turn ON:

Insert a battery and completely close the battery door.


To turn OFF:

Open the battery door until the battery is no longer touching the battery contacts.

Your hearing system has been set to a specific volume level by your hearing care professional. If sounds are generally too loud or too soft, please contact your hearing care professional for advice and adjustment.

Multimemory Settings

Your hearing care professional can set up to four hearing programs for you. These additional programs are accessed by pressing the Multimemory button inward.

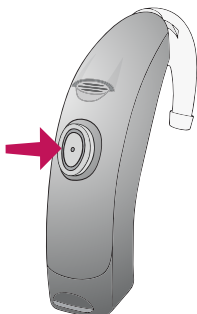

When you press the Multimemory button, you may hear an indicator or a tone series indicating the device has changed to the next program. Your hearing instrument has been set up with the following environments.

Program	Tone	Speech	Environment
1	1 Tone	One	Normal
2	2 Tones	Two	
3	3 Tones	Three	
4	4 Tones	Four	

Operation

Directional Settings

My hearing instrument has directional settings:

Yes

No

Your hearing system has directional microphones to help improve speech understanding in noisy situations.

Your hearing system has been set up with the following directional settings:


Program	Directional Setting		
1	Automatic	Manual	Off
2	Automatic	Manual	Off
3	Automatic	Manual	Off
4	Automatic	Manual	Off

Telephone Use

Your hearing system has a telephone feature that enables you to comfortably use the telephone without removing your hearing instrument.

Automatic Telephone Response (ATR)

Place the telephone handset in a normal position and then shift slightly back. When correctly positioned, you will hear an indicator for the automatic activation of the telephone program. When finished, the hearing system will automatically return to the previous setting.



Operation

Some hearing aid users have reported a buzzing sound in their hearing aids when they are using cell phones, indicating that the cell phone and hearing aid may not be compatible. According to the ANSI C63.19 standard (ANSI C63.19-2006 American National Standard Methods of Measurement of Compatibility Between Wireless Communications Devices and Hearing Aids), the compatibility of a particular hearing aid and cell phone can be predicted by adding the rating for the hearing aid immunity to the rating for the cell phone emissions. For example, the sum of a hearing aid rating of 2 (M2) and a telephone rating of 3 (M3) would result in a combined rating of 5. Any combined rating that equals at least 5 would provide "normal use"; a combined rating of 6 or greater would indicate "excellent performance."

The immunity of this hearing aid is at least M2. The equipment performance measurements, categories and system classifications are based upon the best information available but cannot guarantee that all users will be satisfied.

NOTE: The performance of individual hearing aids may vary with individual cell phones. Therefore, please try this hearing aid with your cell phone or, if you are purchasing a new phone, be sure to try it with your hearing aid prior to purchase. For additional guidance, please ask your cell phone provider for the booklet entitled "Hearing Aid Compatibility with Digital Wireless Cell Phones."

Self Check

Some hearing systems can run a diagnostic test of their own performance. This feature is called Self Check. Your hearing care professional will check the box below if this feature is activated.

Your Self Check feature is activated.

Your Self Check indicator is a:

Speech Indicator (Good, Make appointment)

Tone Indicator

To perform the Self Check:

1. Open and close the battery door three times.
2. Place the hearing system in your ear.
3. Listen for the status indicator.
4. Schedule an appointment with your hearing care professional, if needed.

Operation

Summary of Settings

	Environment	Directional Setting
Program 1	Normal	<input type="checkbox"/> Off <input type="checkbox"/> Automatic <input type="checkbox"/> Manual
Program 2		<input type="checkbox"/> Off <input type="checkbox"/> Automatic <input type="checkbox"/> Manual
Program 3		<input type="checkbox"/> Off <input type="checkbox"/> Automatic <input type="checkbox"/> Manual
Program 4		<input type="checkbox"/> Off <input type="checkbox"/> Automatic <input type="checkbox"/> Manual
Low Battery	—	—
Battery End of Life	—	—
Self Check	—	—
Reminder	—	—

Indicator On	Indicator Type
<input type="checkbox"/> Yes <input type="checkbox"/> No	<input type="checkbox"/> Speech <input type="checkbox"/> 1 Tone
<input type="checkbox"/> Yes <input type="checkbox"/> No	<input type="checkbox"/> Speech <input type="checkbox"/> 2 Tones <input type="checkbox"/> Tone Series
<input type="checkbox"/> Yes <input type="checkbox"/> No	<input type="checkbox"/> Speech <input type="checkbox"/> 3 Tones <input type="checkbox"/> Tone Series
<input type="checkbox"/> Yes <input type="checkbox"/> No	<input type="checkbox"/> Speech <input type="checkbox"/> 4 Tones <input type="checkbox"/> Tone Series
<input type="checkbox"/> Yes <input type="checkbox"/> No	<input type="checkbox"/> Speech <input type="checkbox"/> Tone Series
<input type="checkbox"/> Yes <input type="checkbox"/> No	<input type="checkbox"/> Speech <input type="checkbox"/> Sustained Tone
<input type="checkbox"/> Yes <input type="checkbox"/> No	<input type="checkbox"/> Speech <input type="checkbox"/> Tone Series
<input type="checkbox"/> Yes <input type="checkbox"/> No	<input type="checkbox"/> Speech <input type="checkbox"/> Tone Series

Hearing System Care

Instrument Care

My hearing instrument has:

- Standard tubing
- Thin tubing


Do your best to keep your hearing instrument clean at all times. Heat, moisture and foreign substances can result in poor performance.

- Use a cleaning brush or soft cloth to clean debris from around the switches, microphone and battery compartment
- Never use water, solvents, cleaning fluids or oil to clean your instrument


Standard Tubing

1. Separate the Custom Earmold from the BTE by gently pulling the tubing away from the earhook.
 - Use a soft, damp cloth or a cleaning brush to clean debris from the Custom Earmold

- Wash the Custom Earmold with warm soapy water
 - Never use solvents
2. Slide the Custom Earmold tubing onto the BTE earhook when completely dry.



1




2

Your hearing care professional can provide further information on additional maintenance procedures for your hearing system if needed.

Hearing System Care

Thin Tubing

1. Unscrew the tubing from the tip of the hearing instrument.

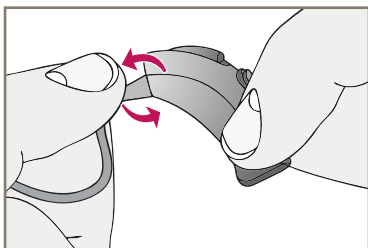

1

2. Thread the cleaner through the tubing starting at the end just removed from the hearing instrument until it extends from the other end of the tubing.
3. Brush the debris off prior to removing the cleaner.

4. Clean the Earbud/Eartip with a dry cloth or brush.
5. If necessary, the Earbud/Eartip may be washed in warm, soapy water. Remove the Earbud/Eartip from the tubing prior to washing. Allow the Earbud/Eartip to dry overnight.

Hearing System Care

Helpful Hints

- Make sure the Custom Earmold and tubing are completely dry before reconnecting to your hearing instrument earhook
- When not wearing your hearing system, open the battery door to allow any moisture to evaporate
- When not in use, remove the batteries completely; place your hearing system in the storage container and store:
 - In a dry, safe place
 - Away from direct sunlight or heat to avoid extreme temperatures
 - Where you can easily find them
 - Safely out of reach of pets and children
- Do not take apart your hearing instruments or insert the cleaning tools inside them

Service and Repair

If, for any reason, your hearing system does not operate properly, do NOT attempt to fix it yourself. Not only are you likely to violate any applicable warranties or insurance, you could easily cause further damage.

Should your hearing system fail or perform poorly, check the guide on the next page for possible solutions. If problems continue, contact your hearing care professional for advice and assistance. He or she is able to solve many common problems right in his or her office or clinic.

Hearing System Care

Troubleshooting Guide

SYMPTOM	POSSIBLE CAUSES	SOLUTIONS
Not Loud Enough	Low battery	Replace battery
	Blocked earmold/tubing/earbud	Remove blockage and clean
	Hearing change	Contact your hearing care professional
	Debris buildup	Clean both microphone and receiver with brush
Inconsistent Performance	Low battery	Replace battery
	Blocked earmold/tubing/earbud	Remove blockage and clean
Unclear, Distorted Performance	Low battery	Replace battery
	Blocked earmold/tubing/earbud	Remove blockage and clean
	Defective hearing instrument	Contact your hearing care professional

Hearing System Care

SYMPTOM	POSSIBLE CAUSES	SOLUTIONS
Dead	Low battery	Replace battery
	Blocked earmold/tubing	Remove blockage and clean
	Crimped tubing	Contact your hearing care professional

Tips for Better Communication

Your hearing care professional will recommend an appropriate schedule to help you adapt to your new hearing system. It will take practice, time and patience for your brain to adapt to the new sounds that your hearing system provides. Hearing is only part of how we share thoughts, ideas and feelings. Reading lips, facial expressions and gestures can help the learning process and add to what amplification alone may miss.

Please review the following simple communication tips:

For You

- Move closer to and look at the speaker
- Sit face-to-face in a quiet room
- Try different locations to find the best place to listen
- Minimize distractions
- Background noises may be frustrating at first; remember, you have not heard them for a while
- Let others know what you need; keep in mind that people cannot "see" your hearing loss

Tips for Better Communication

- Develop realistic expectations of what your hearing instruments can and cannot do
- Better hearing with hearing instruments is a learned skill combining desire, practice and patience

For Your Family and Friends

Your family and friends are also affected by your hearing loss. Request that they:

- Get your full attention before beginning to speak
- Look at you or sit face-to-face in a quiet room
- Speak clearly and at a normal rate and level; shouting can actually make understanding more difficult
- Rephrase rather than repeat the same words; different words may be easier to understand
- Minimize distractions while speaking

Notes

Required Information

The following additional information is provided in compliance with U.S. Food and Drug Administration (FDA) regulations:

WARNING TO HEARING AID DISPENSERS. A hearing aid dispenser should advise a prospective hearing aid user to consult promptly with a licensed physician (preferably an ear specialist) before dispensing a hearing aid if the hearing aid dispenser determines through inquiry, actual observation, or review of any other available information concerning the prospective user, that the prospective user has any of the following conditions:

- i. Visible congenital or traumatic deformity of the ear.
- ii. History of active drainage from the ear within the previous 90 days.
- iii. History of sudden or rapidly progressive hearing loss within the previous 90 days.
- iv. Acute or chronic dizziness.
- v. Unilateral hearing loss of sudden or recent onset within the previous 90 days.
- vi. Audiometric air-bone gap equal to or greater than 15 decibels at 500 Hertz (Hz), 1,000 Hz and 2,000 Hz.
- vii. Visible evidence of significant cerumen accumulation or a foreign body in the ear canal.
- viii. Pain or discomfort in the ear.

RF IMMUNITY LEVEL. This hearing aid has a cell phone immunity rating of M3. A hearing aid compatible cell phone must carry a rating of M2 or higher to work with this hearing aid. Please consult your cell phone specification for the cell phone immunity rating.

IMPORTANT NOTICE FOR PROSPECTIVE HEARING AID USERS.

Good health practice requires that a person with a hearing loss have a medical evaluation by a licensed physician (preferably a physician who specializes in diseases of the ear) before purchasing a hearing aid. Licensed physicians who specialize in diseases of the ear are often referred to as otolaryngologists, otologists, or otorhinolaryngologists. The purpose of the medical evaluation is to assure that all medically treatable conditions that may affect hearing are identified and treated before the hearing aid is purchased.

Following the medical evaluation, the physician will give you a written statement that states that your hearing loss has been medically evaluated and that you may be considered a candidate for a hearing aid. The physician will refer you to an audiologist or hearing aid dispenser, as appropriate, for a hearing aid evaluation.

The audiologist or hearing aid dispenser will conduct a hearing aid evaluation to assess your ability to hear with and without a hearing aid. The hearing aid evaluation will enable the audiologist or dispenser to select and fit a hearing aid to your individual needs.

If you have reservations about your ability to adapt to amplification, you should inquire about the availability of a trial-rental or purchase-option program. Many hearing aid dispensers now offer programs that permit you to wear a hearing aid for a period of time for a nominal fee after which you may decide if you want to purchase the hearing aid.

Federal law restricts the sale of hearing aids to those individuals who have obtained a medical evaluation from a licensed physician. Federal law permits a fully informed adult to sign a waiver statement declining the medical evaluation for religious or personal beliefs that preclude consultation with a physician. The exercise of such a waiver is not in your best health interest and its use is strongly discouraged.

A hearing aid will not restore normal hearing and will not prevent or improve a hearing impairment resulting from organic conditions. In most cases infrequent use of a hearing aid does not permit a user to attain full benefit from it.

CHILDREN WITH HEARING LOSS. In addition to seeing a physician for a medical evaluation, a child with a hearing loss should be directed to an audiologist for evaluation and rehabilitation since hearing loss may cause problems in language development and the educational and social growth of a child. An audiologist is qualified by training and experience to assist in the evaluation and rehabilitation of a child with a hearing loss.

NuEar
6769 Mesa Ridge Road
Suite 100
San Diego, CA 92121
800.626.8327
858.450.9972

www.NuEar.com

